FUJI MASSAGE CHAIR

User operation manual

Model: Waikiki II

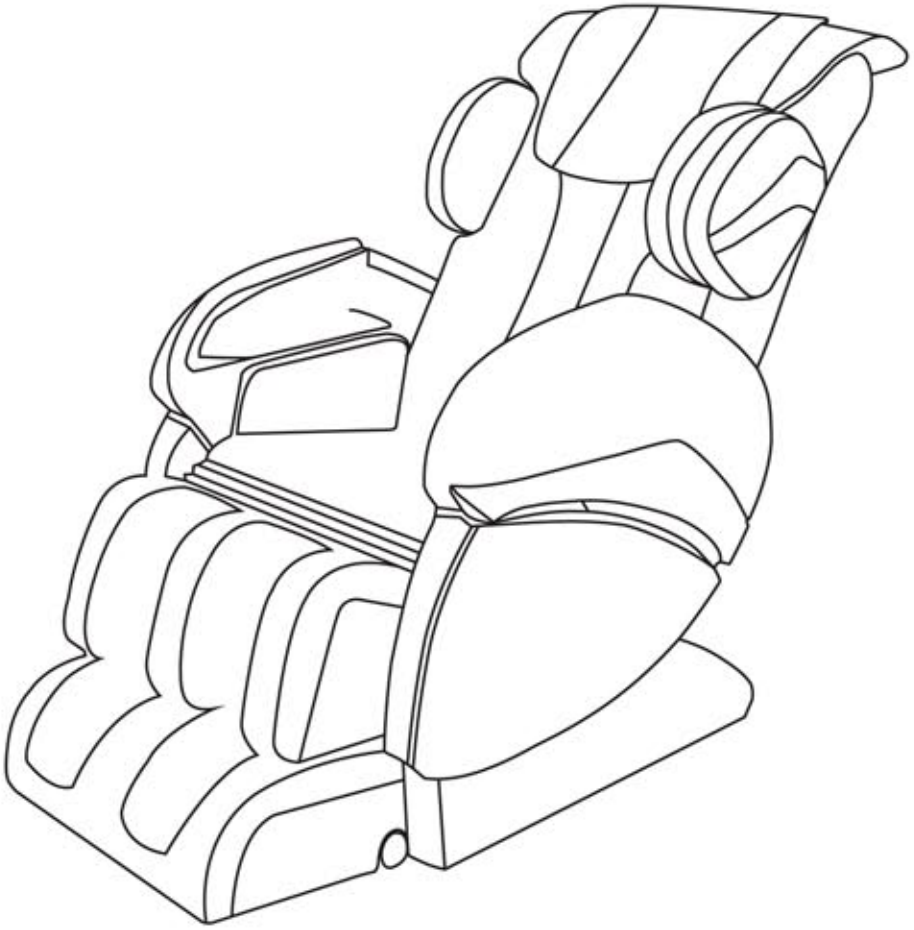

CONTENTS

CONTENTS 1

SAFETY INTRODUCTION 2

CONTROLLER INSTRUCTION 5

PREPAPATION BEFORE USE 6

ASSEMBLY METHOD 7

PRODUCT INSTALLATION 8

ARMREST DISASSEMBLY METHOD 9

PREPARATION BEFORE MASSAGE 10

NAME OF EACH PART 11

MAINTAINANCE 12

ILLUSTRATION 13

TROUBLESHOOTING 14

TROUBLESHOOTING

If abnormal sounds or movements are observed, please power off the massage chair by turning off the main power switch, and removing the plug from the electric outlet. Please contact the customer service department for further assistance.

Problem	Solution
The massage chair is connected to power but is not functioning.	1. Check to see if plug is inserted properly, or if power outlet is functioning properly. 2. Check to see if the main power switch is in the "ON" position.
The remote controller is responding, but the massage chair is not functioning.	The massage chair may have automatically shut down due to overheating protection devices. Please turn off the power and allow the chair to cool off for 30-50 minutes.
Both the remote controller and massage chair are not responding.	The massage chair automatically goes into idle mode when a massage program is completed. Please press the power button again to turn on the chair.

Specification

Product Name	Massage Chair
Model	
N.W./G.W.	104Kg/90Kg
Rated Power	240V~120W
Outer Package	1300*800*850mm
Rated Time	15min

SAFETY INTRODUCTION

A. Usage environment

1. Do not use the chair in an excessively humid or dusty environment, as this may cause electrical shock or malfunction.
2. Do not use the chair in room temperature higher than 40^{0}C.
3. Do not expose the chair to heaters, stoves or direct sunlight.
4. Do not use the chair where environmental temperature changes sharply.
5. Do not use the chair where there is not enough space or good ventilation.
6. Do not insert any object into or around the gaps of massage chair.

CAUTIONS

Should you use the chair in a cold room, do not increase the room temperature abruptly. It is recommended that you increase the temperature gradually to a normal level. In the event that the chair is stored in a cold place and is being brought into a warm place, it is advisable to use it one hour later. Machine malfunction may ensue when a cold machine is being used in warm room suddenly.

B. Unsuitable users

If you are under medical treatment or having any of following symptoms, please consult your doctor before use:
- Those who are suffering from heart diseases.
- Those who are suffering from malignant tumors.
- Those who are under medical care or are feeling unwell.
- Women who are pregnant or menstruating
- Those who are under medical rest or rest-cure ordered by doctors.
- Those with back problems such as spinal disorders, bent or abnormal spinal conditions caused by past accidents or illnesses.
- Those who have high fever
- Those who are suffering from osteoporosis.
- Those who are injured or have skin disease.
- Children under 12 years old or people mentally unbalanced without being supervised.

CAUTIONS

This machine is not recommended for people with disabilities (including children).

ILLUSTRATION

Acupressure Point Massage Instruction

Every Vertebra is related with the health, for example:

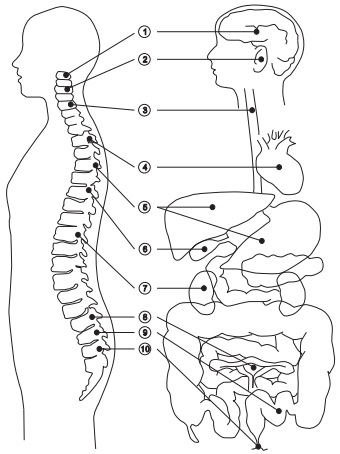

1. The first bone of neck vertebra diagnoses headache.
2. The third bone of neck vertebra diagnoses hard of hearing.
3. The fifth bone of neck vertebra diagnoses bronchus.
4. The second bone of chest vertebra diagnoses cardiopathy.
5. The fourth bone of chest vertebra diagnoses liver disease and tummy bug.
6. The ninth bone of chest vertebar diagnoses chololith.
7. The sixth bone of chest vertebra diagnoses nephropathy.
8. The third bone of waist vertebra diagnoses constipation and back pain.
9. The fifth bone of waist vertebra diagnoses hemorhoid.

SAFETY INTRODUCTION

C. Safety precautions

1. To ensure safe and correct use of the chair, do not operate the chair without carefully reading of this operational manual.
2. Do not use the chair in combination with other therapeutic equipment, electric blankets, etc, as it may result in ineffectiveness or injury.
3. Do not allow children or pets to play around the chair, i.e. behind the backrest, under the seat ,there is risk of injury and damage.
4. Do not rest or place heavy objects on the footrest or backrest. It may result in machine malfunction or injury to the user should these objects topple.
5. Do not use the chair when the body is wet.
6. Do not operate the chair with wet hands.
7. Prolonged application of massage at a position of your body may result in excessive stimulation and may be counter-effective.
8. Do not insert your hand or foot into or at the paths of the massage nodes during the operation of the chair, as it may cause injury.
9. Do not use the chair with1 hour after meal .
10. If the power is lost during operation, please switch the power off and unplug from outlet to avoid any damages.
11. Do not stand, sit or jump on backrest, armrest and footrest to prevent injury and damage to massage chair.
12. Do not fall asleep on the massage during operation.
13. Always check the machine condition before operating the chair.
14. If water is spilled on the machine,continuous usage under these conditions may result in electrical shock.
15. If abnormal or severe pain is felt during massage, stop operation immediately and consult your doctor.
16. If you detect any malfunction or any other abnormal condition during operation, stop operation and contact Dr.Care Service Centre for inquiries.
17. Do not massage any swollen or inflamed part of your body.
18. Do not use this machine as a substitute for medical treatment.
19. Senior citizens are not encouraged to apply the Zero Gravity function on this machine.

CAUTIONS

1. You may place a blanket or towel over the backrest if you prefer a softer massage.
2. Using the massage chair as a bed is not recommended.
3. Do not apply massage directly on the head, joints of elbows and knees, breasts or abdomen.

MAINTENANCE

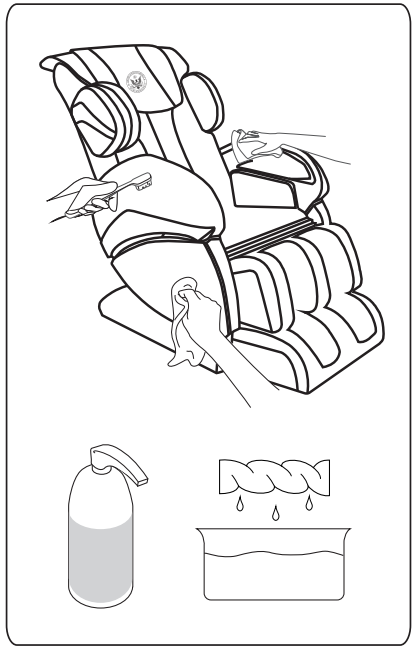

- Use dry cloth to wipe sweat and other besmirch.

- If besmirch is serious, please use **diluted liquid soap solution to wipe the chair.**

- If besmirch is very serious, brush the chair lightly and carefully.

- Please make the chair airy.

- Shout **the power** off and pull out the plug before clean**ing** the chair.**D**o not touch the plug with wet hand**s.**

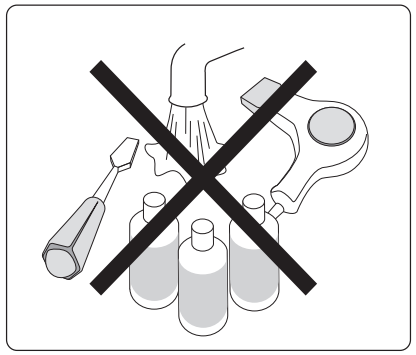

- Prohibit to use water to clean the chair.

- Do not dry the chair with **blow dryer.**

- **Do not** use alcohol, benzene wash etc.

SAFETY INTRODUCTION

4. Suggested per usage time is 15 minutes. Suggested per usage time on a partic lar body part is 5 minutes.
5. Do not use the machine if the centre of the upholstery is torn. Remove the AC plug from the electrical outlet immediately. Continuous usage of the chair in this condition may cause injury to the user or may lead to electric shock.

D. Assemble and repair of the chair

1. Do not disassemble the back cover of chair to avoid electrical shock.
2. The chair must only be serviced or repaired by Dr.Care Service Centre.
   You must not disassemble or repair it by yourself.
3. Do not try to replace the machinery parts by non-Dr.Care provided spare parts

E. Things to take note on power plug and cord

1. Check the voltage corresponds with the specifications indicated for the chair. (only for alternative current)
2. Do not disconnect the AC plug from electrical outlet roughly.
3. Do not connect or disconnect the AC plug from the electrical outlet with wet hands. It may cause electrical shock or machine malfunction.
4. When disconnecting the AC plug, pull it out by holding on the plug, not pulling on the cord.
5. Always switch off the power switch after operation and remove the power plug from outlet.
6. Make sure the power plug is plug-in to outlet properly to avoid electrical shock.
7. Do not move the machine by pulling power cord.
8. Do not place the AC cord under the chair as it may damage the cord and may cause fire or electrical shock.
9. Do not operate the chair or tamper with a damage cord or electrical plug. Contact Dr.Care Service Centre for inspection. Use only attachments recommended by Dr.Care.
   Do not use the chair if the electrical outlet is excessively loose.

NAME OF EACH PART

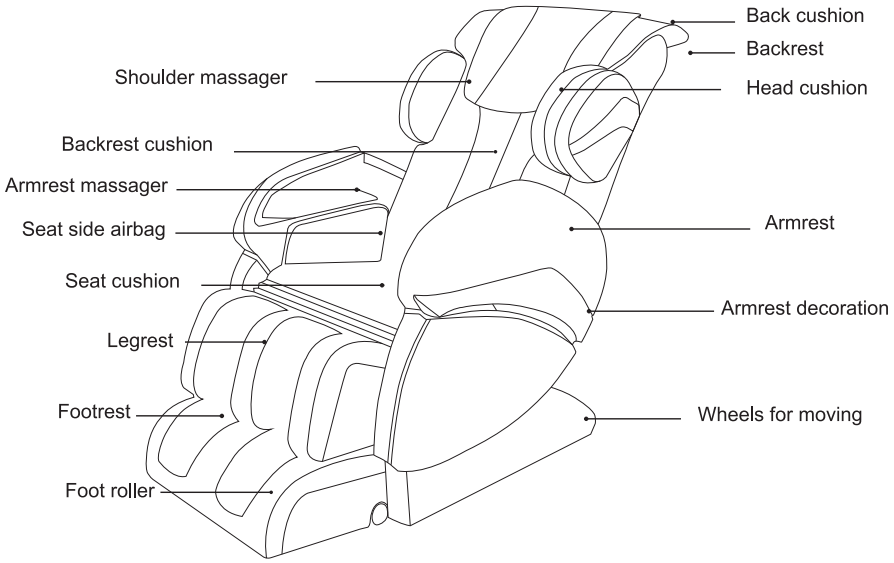

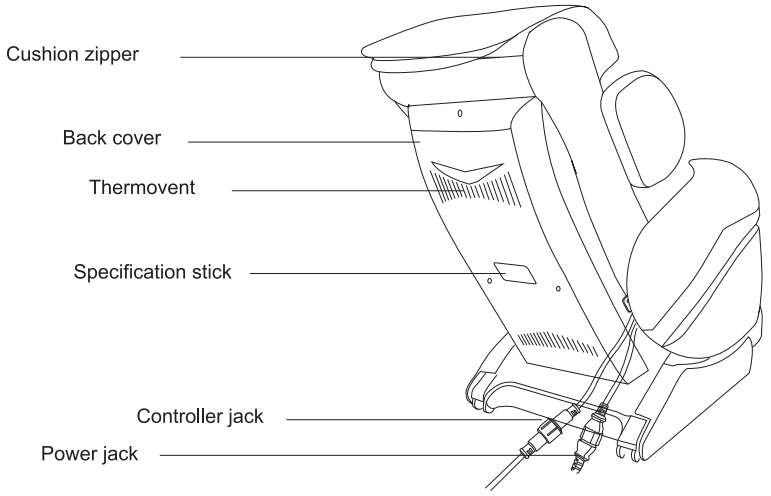

CONTROLLER INSTRUCTION

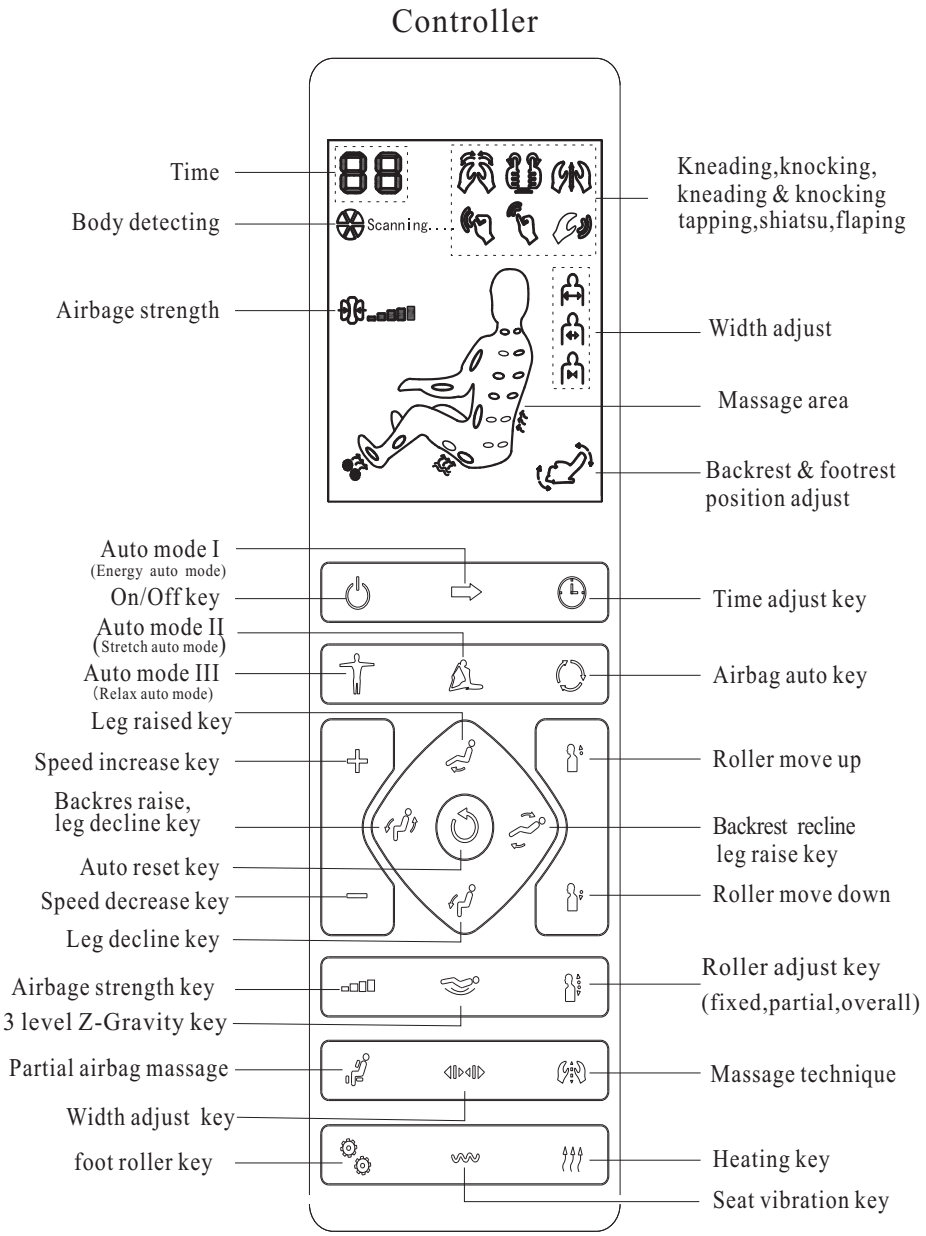

PREPARATION BEFORE MASSAGE

1. Power On

1. Connect AC plug to an electrical outlet and insert the connector of the power cord to the electrical inlet (located on the left side of backrest).
2. Switch on the main switch located on the left side of backrest.
3. Press the power key on the remote controller to operate the chair. The LCD display screen on the remote controller will light up.

Warning

1. Ensure that the AC cord is not placed under the foot of the chair.
2. Ensure that all switches are at the OFF position (including the main switch) before the AC plug is connected to an electrical outlet.
3. If the backrest rollers are located at the middle of the backrest upon termination of the previous operation, they will return to their original position when the main switch is switch on agian.

2. How to operate the chair

1. Ensure the footrest is at the lowest position.
2. Ensure the 4 real-touch massage rollers are position at "storage positon" (the upper part of the backrest) before sitting on the chair. If you find the rollers are not projecting outward from the storage position, please switch off the power right away, so that the rollers will return to the storage positon.

3. After use

1. With the auto-timer function, the chair will stop automatically after 15 minutes of operation. Please switch off the main switch after use.
2. Ensure the main switch is off and disconnect the AC plug from electrical outlet after use to avoid any malfunction of the chair or accidents to children.

PREPARATION BEFORE USE

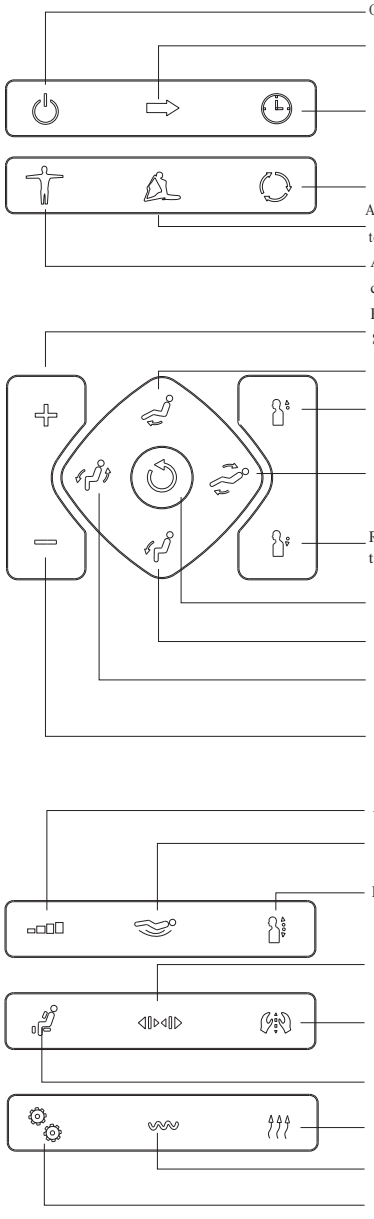

ON/OFF key: Press this button,5 minutes full body massage rapid experience automatically start.

Auto mode I: Energy auto mode, rhythmic massage benefits accelerating body metabolism. Press again to close the mode

Time adjust key: During massage, press this button to change time in 15 minutes、20 minutes、30 minutes in sequence.

Airbag auto key: Press this button, full body airbag massage function start.

Auto mode II: Stretch auto mode，based on normal massage types,combine stretching method, to relieve whole body meridian. Press again to close the mode.

Auto mode III: Relax auto mode, the whole body relieving massage mode, combined different strength and speed, suitable for alleviating fatigue. Press again to close the mode.

Speed increase key: total of 3 level in sequence.

Leg raised key: Press this button to raise calfrest,press again to stop.

Roller move up: Press this button to raise back massage unit press again to stop.

Backrest recline, leg raise key: Press this button to lower backrest and raise calfrest. Press again to stop.

Roller move down: Press this button to lower back massage unit press again to stop.

Auto reset: Press this button for calfrest and backrest to return to default positions.

Leg decline key: Press this button to lower calfrest，press again to stop.

Backrest raise,leg decline key: Press this button to lower calfrest and raise backrest , Press again to stop.

Speed decrease: total of 3 levels.

Airbag strength key: 3 levels in sequence.

3 level Z-Gravity key: Press this button for 3 adjustments of zero gravity.

Roller adjust: Roller adjustment activate button. press this button before press (point,part,overall)

Width adjust key: Press this button to adjust the back massage unit (wide , medium, narrow) 3 kind of width.

Massage technique: Kneading , knocking, kneading and knocking, pressing , tapping, shiatsu.6 kind of massage technique adjustment.

Partial airbag massage : Armrest ,seat, leg air bag massage adjustment.

Heating : Press button to start, press again to stop.

Seat vibration: Press button to start, total 3 levels of speed in sequence.

Foot roller massage: total 3 levels of speed in sequence.

Armrest disassembly method

A.Assembly the armrest when backrest is erect. Pls according to the A,B,C order to assemble

B.The armrest shaft assemble.
(Insert the two iron shafts into the corresponding hole of base)

C.Fix the screws
(After the screws fixed, inset the screw and tighten the screws)

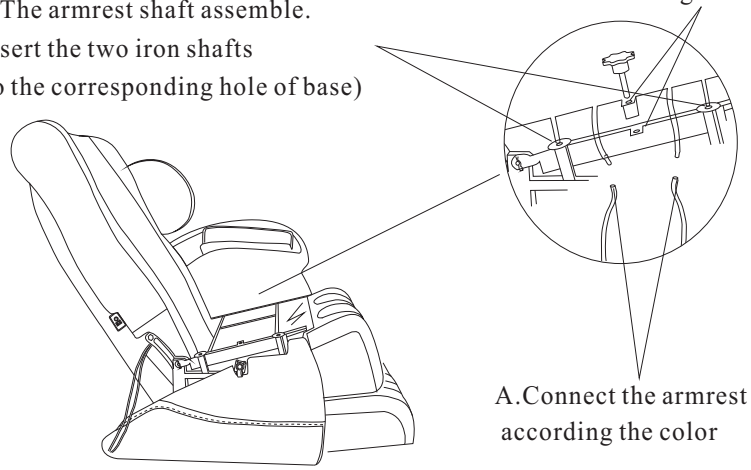

A.Connect the armrest airbag tube according the color

Massage chair setting method

Around the massage chair should has enough space, and lay on smooth ground

Remark: When the backrest is low and calfrest is raised, there need more than 50cm space in front and more than 10cm space behind the chair to avoid crash.

Remark: Suggest roll out a base wad under the chair to avoid damage of the ground and carpet.

Remark: To avoid leather damage or color change, please don't put the chair to the sun or in high temperature place.

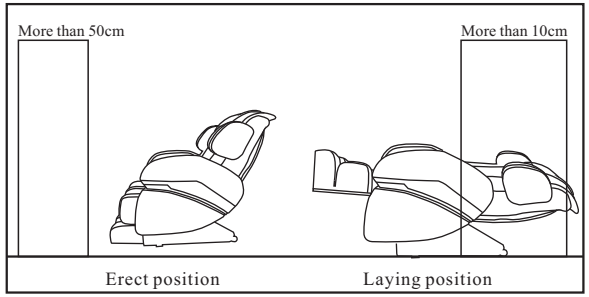

Massage chair moving method

Lift the backrest and push the whole chair by hands

Attentions

1.Don't move it with people or object on it, in case of turnover.
2.Don't move the chair or drag wheels on ground that is easy to scratch.
3.Please don't take up the seat part, leg part and shoulder part when moving the chair.
4.Please notice its weight when lifting the calfrest.

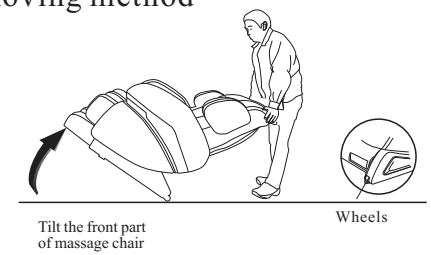

ASSEMBLY METHOD

Massage chair and components

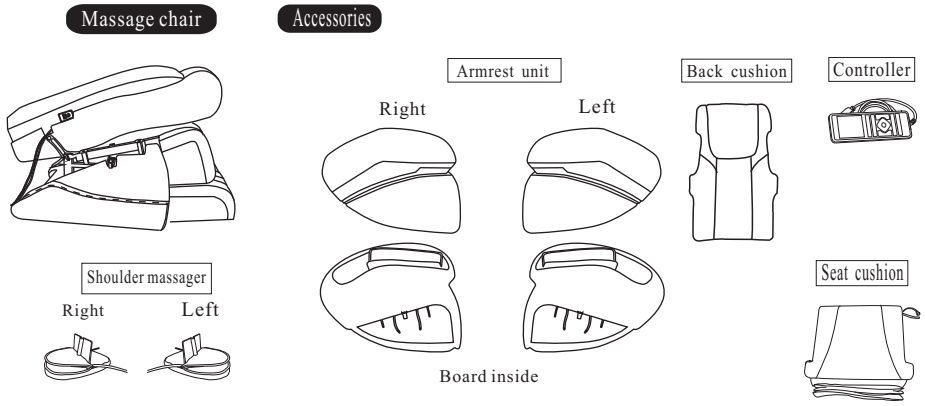

Remark
Please use the appointed spare parts in the carton.

Backrest assembly and fold method

Lift the backrest follow the arrow direction, and make sure the locking structure(part inside the circle) is fixed (you should hear a clicking sound)
* Notice: lift up softly and fold slowly.

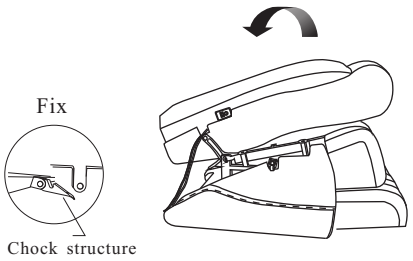

Press the locking structure under the backrest(Part inside the circle),and push backrest forward.
*Please notice: do not fold the chair suddenly.
*Please do not lower the backrest when the chair's shoulder and armrest are installed.

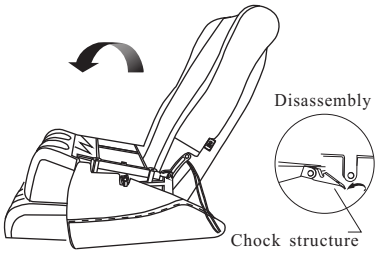

PRODUCT INSTALLATION

Shoulder installation method

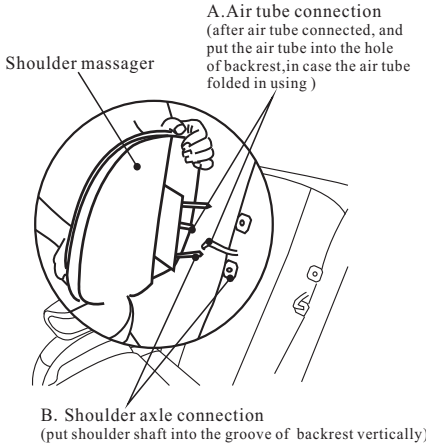
A.Air tube connection
(after air tube connected, and put the air tube into the hole of backrest,in case the air tube folded in using)
Shoulder massager
B. Shoulder axle connection
(put shoulder shaft into the groove of backrest vertically)

Backrest cushion installation method

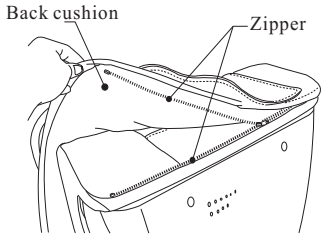

Remark
Assemble the other side in the same way.
Disassemble according the installation method.

Seat cushion installation method

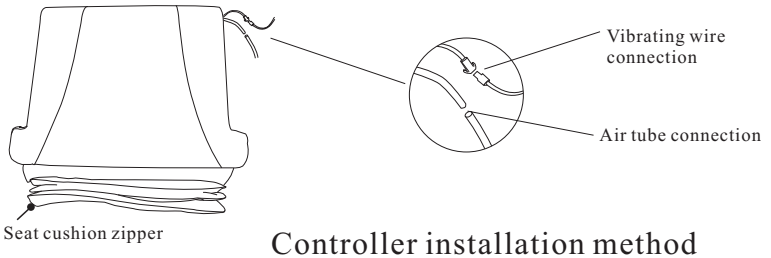

Controller installation method

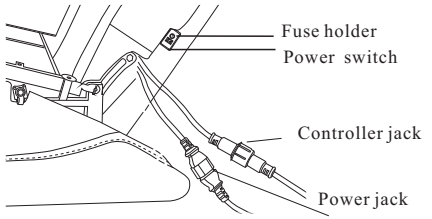

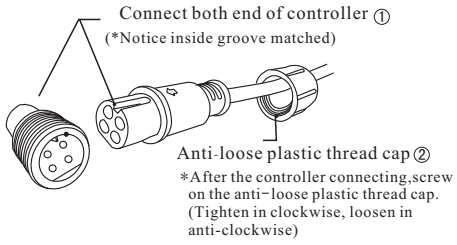
Connect both end of controller ①
(*Notice inside groove matched)
Anti-loose plastic thread cap ②
*After the controller connecting,screw on the anti-loose plastic thread cap. (Tighten in clockwise, loosen in anti-clockwise)